

FIG. 1

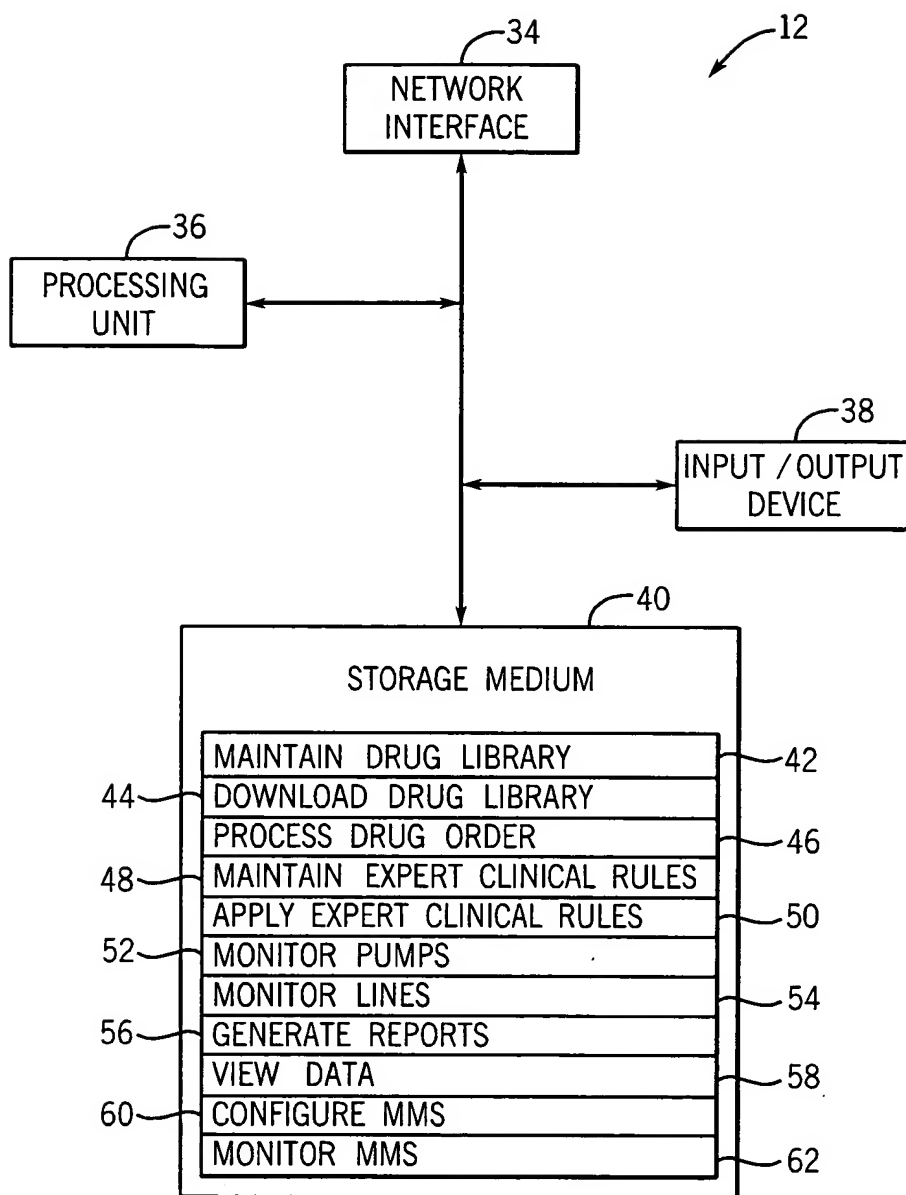


FIG. 2

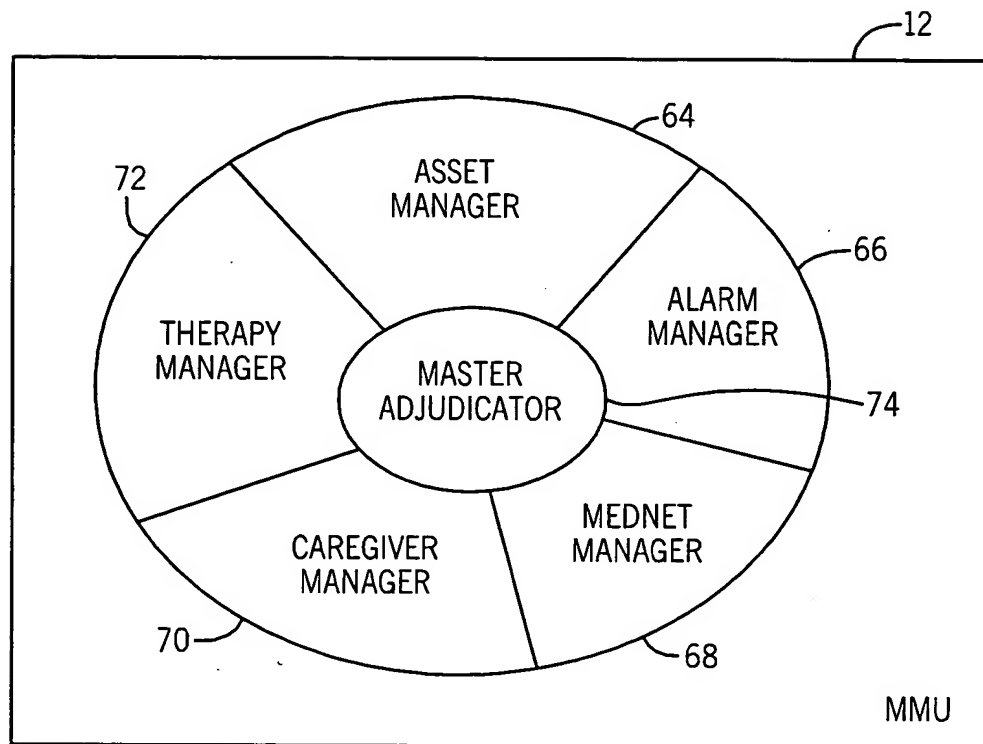


FIG. 3

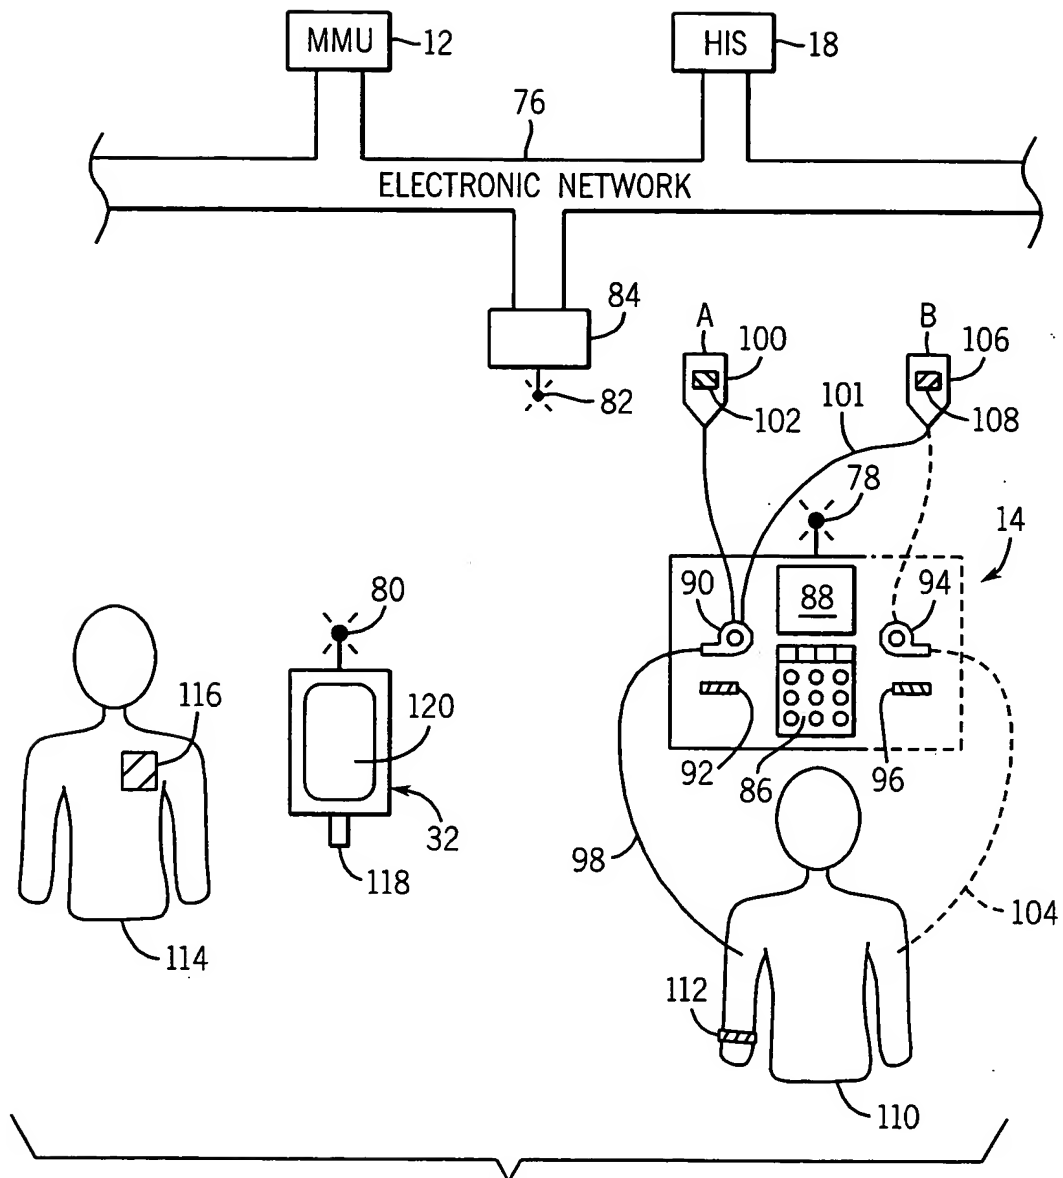


FIG. 4


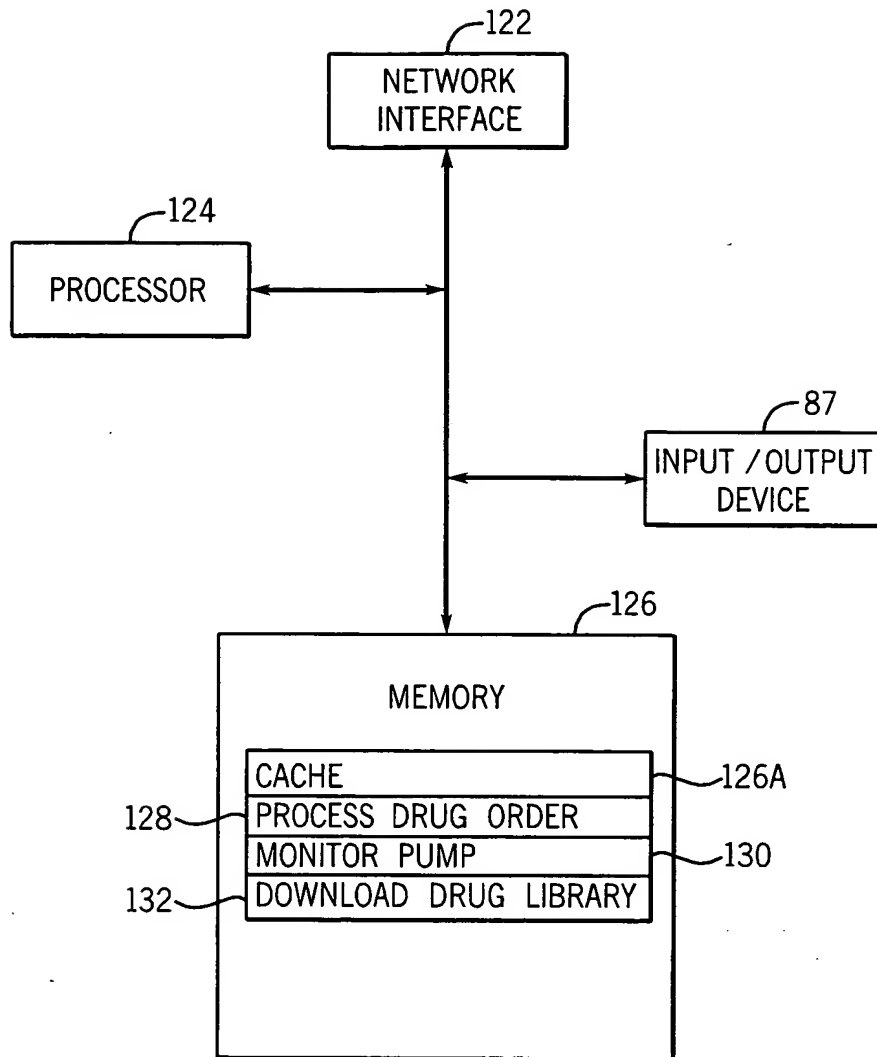


FIG. 4A

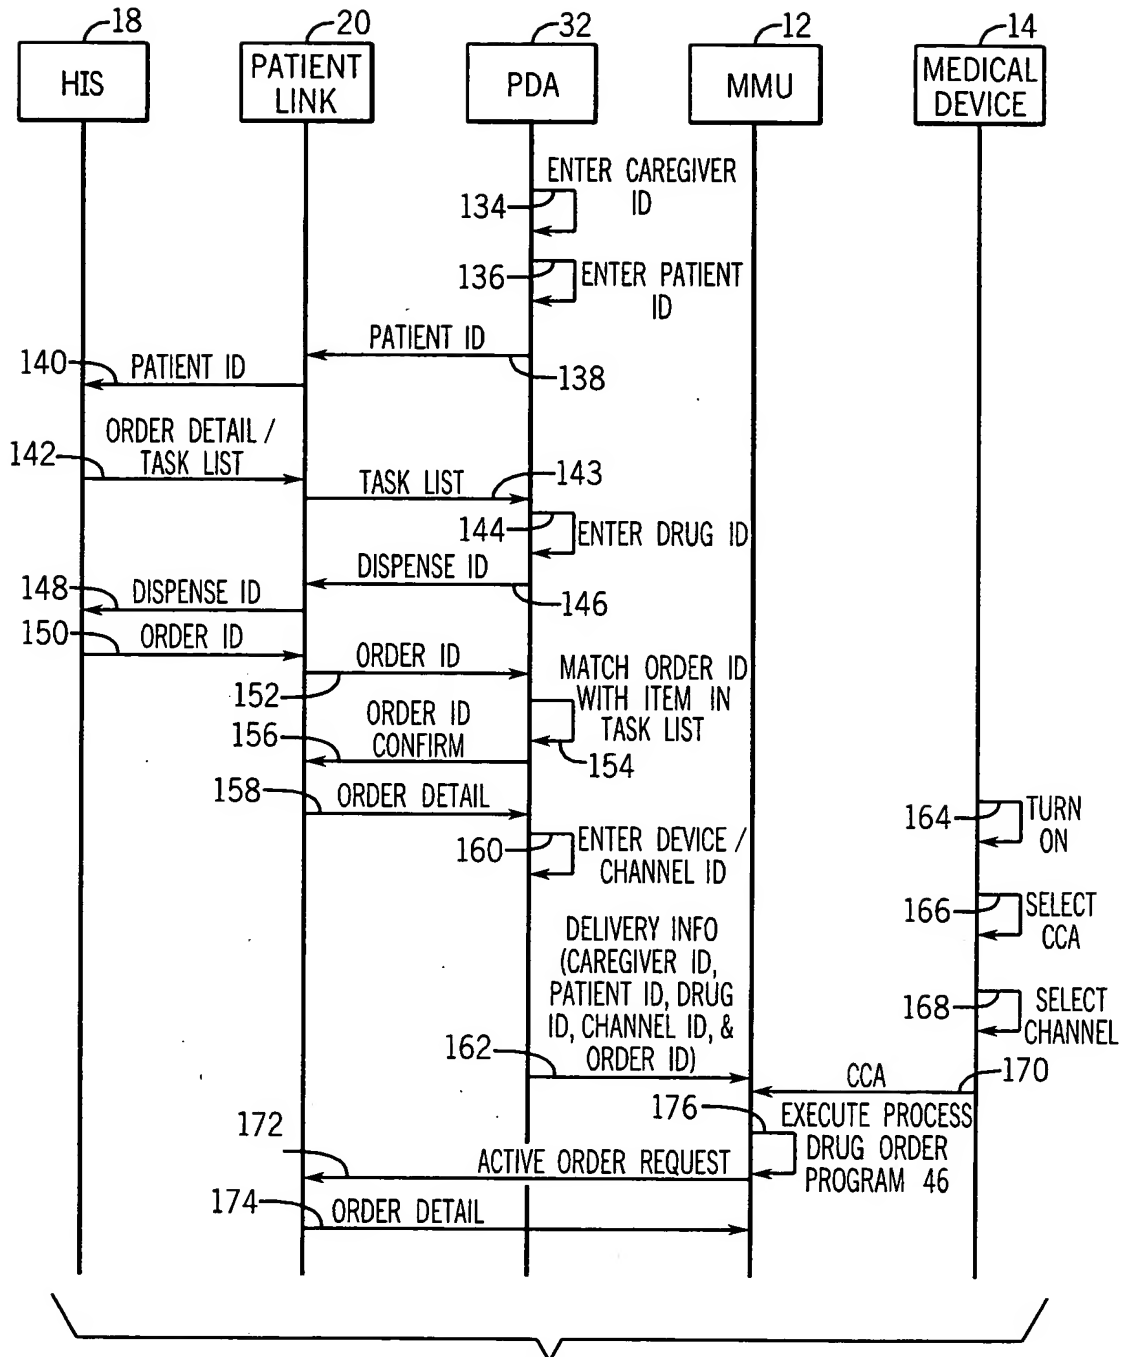

TO FIG. 5A

FIG. 5


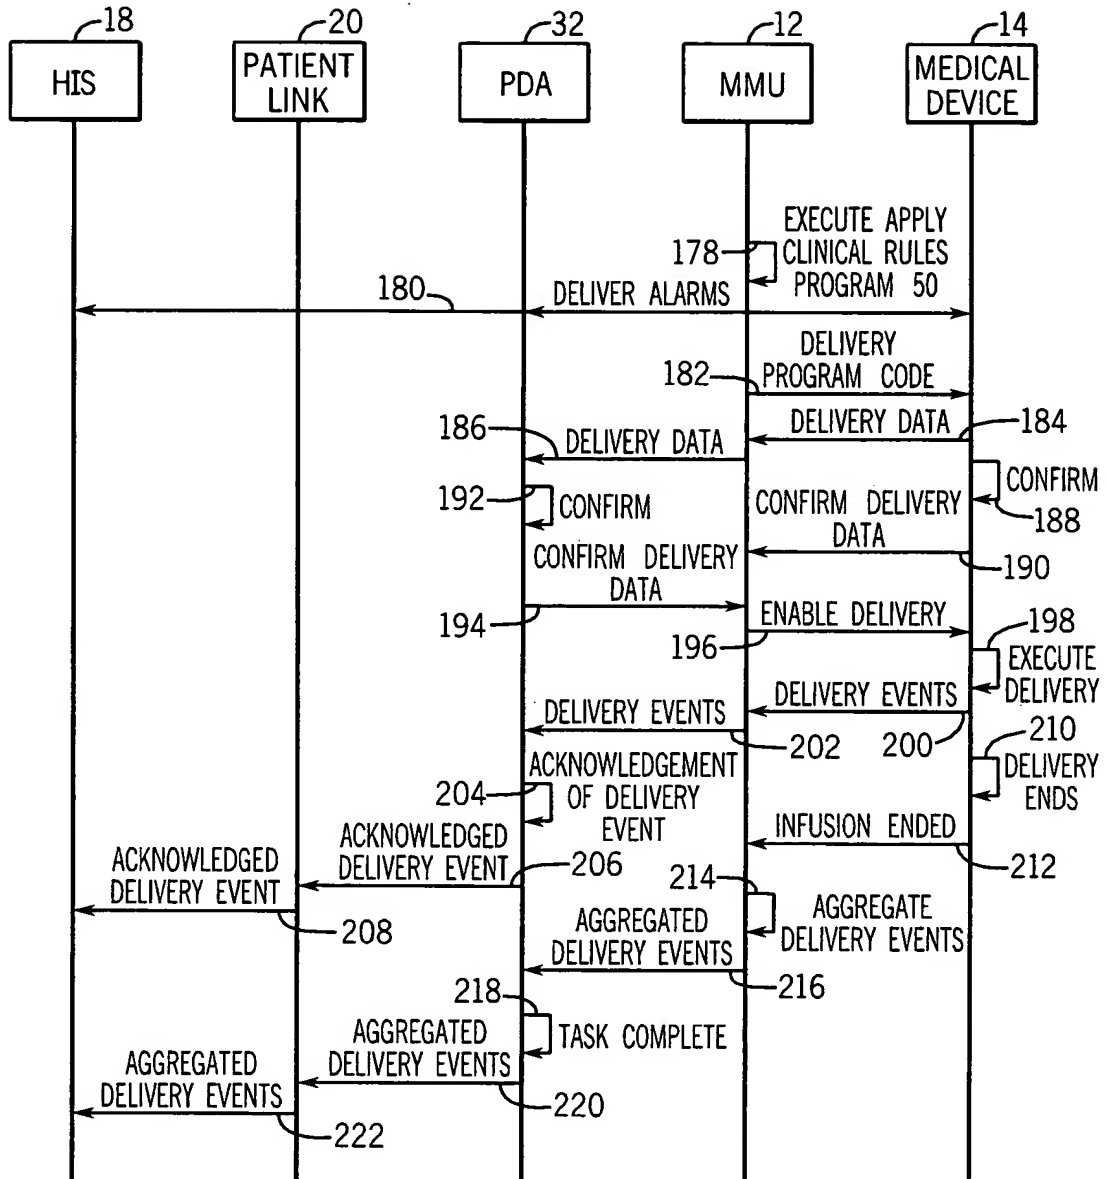


FIG. 5A

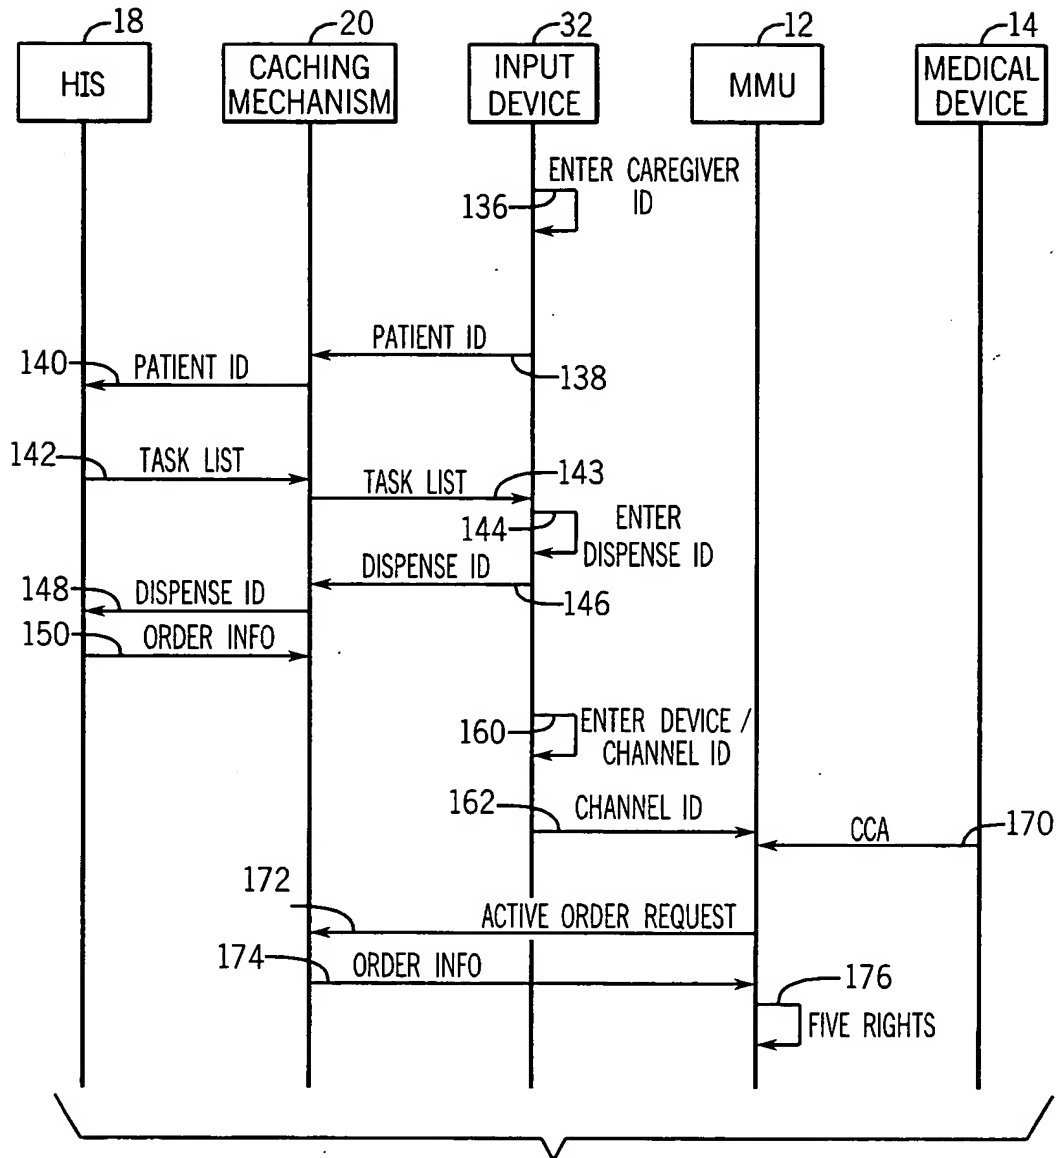

TO FIG. 6A

FIG. 6

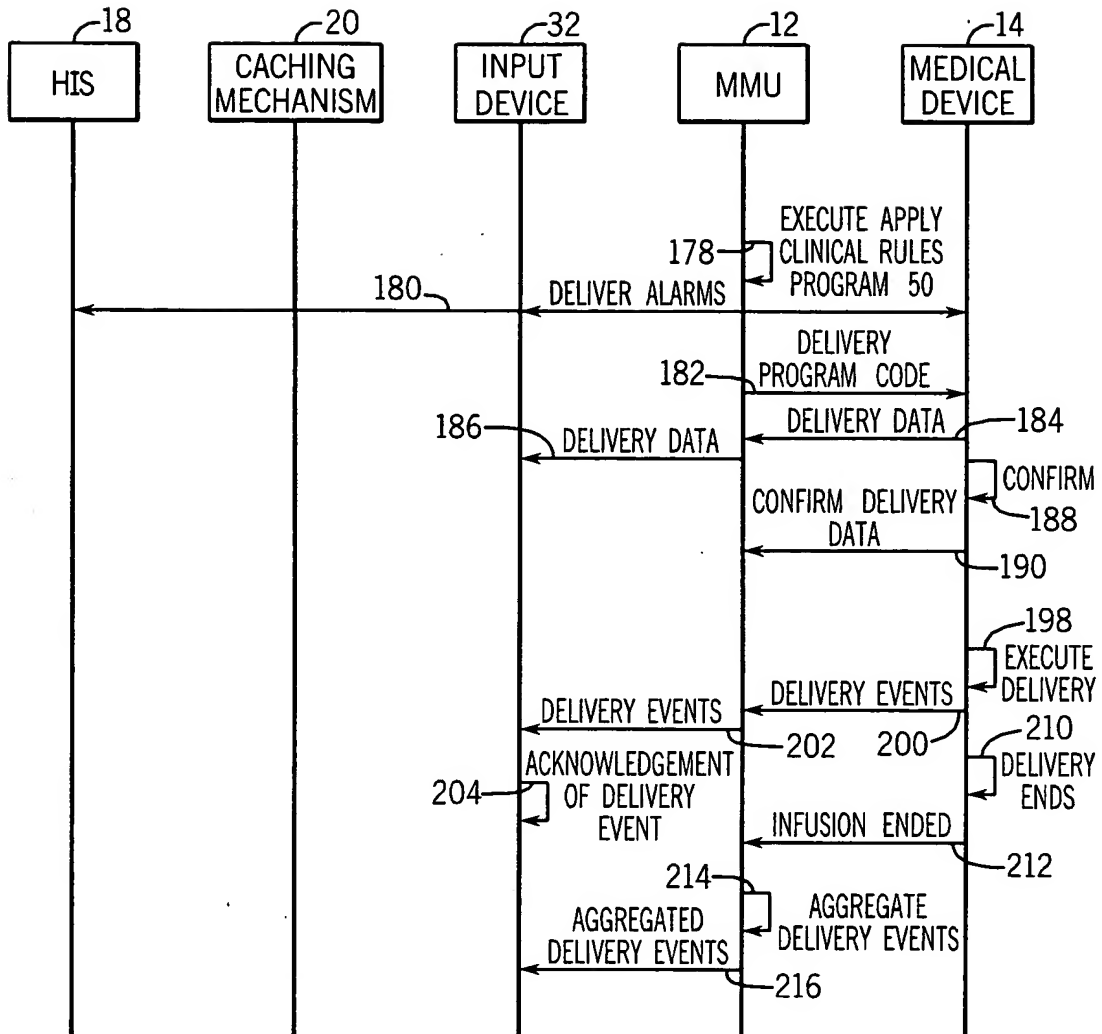


FIG. 6A

133B

:PDAAPPL01_2004

File Zoom Tools Help

User name:

Password:

123	1	2	3	4	5	6	7	8	9	0	-	=	←
Tab	q	w	e	r	t	y	u	i	o	p	[]	
CAP	a	s	d	f	g	h	j	k	l	;	,		
Shift	z	x	c	v	b	n	m	,	.	/		↵	
Ctl	a ã	`	/						↓	↑	-	→	

Quit



 

FIG. 7

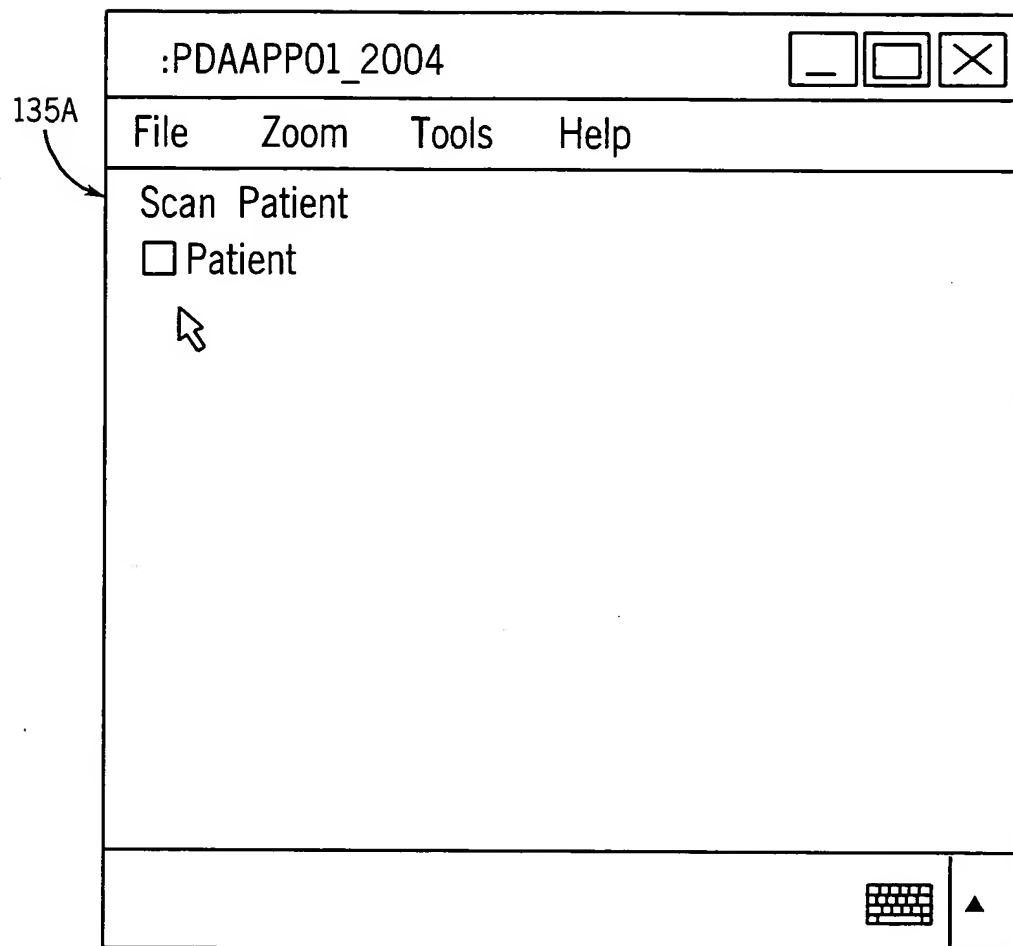


FIG. 8

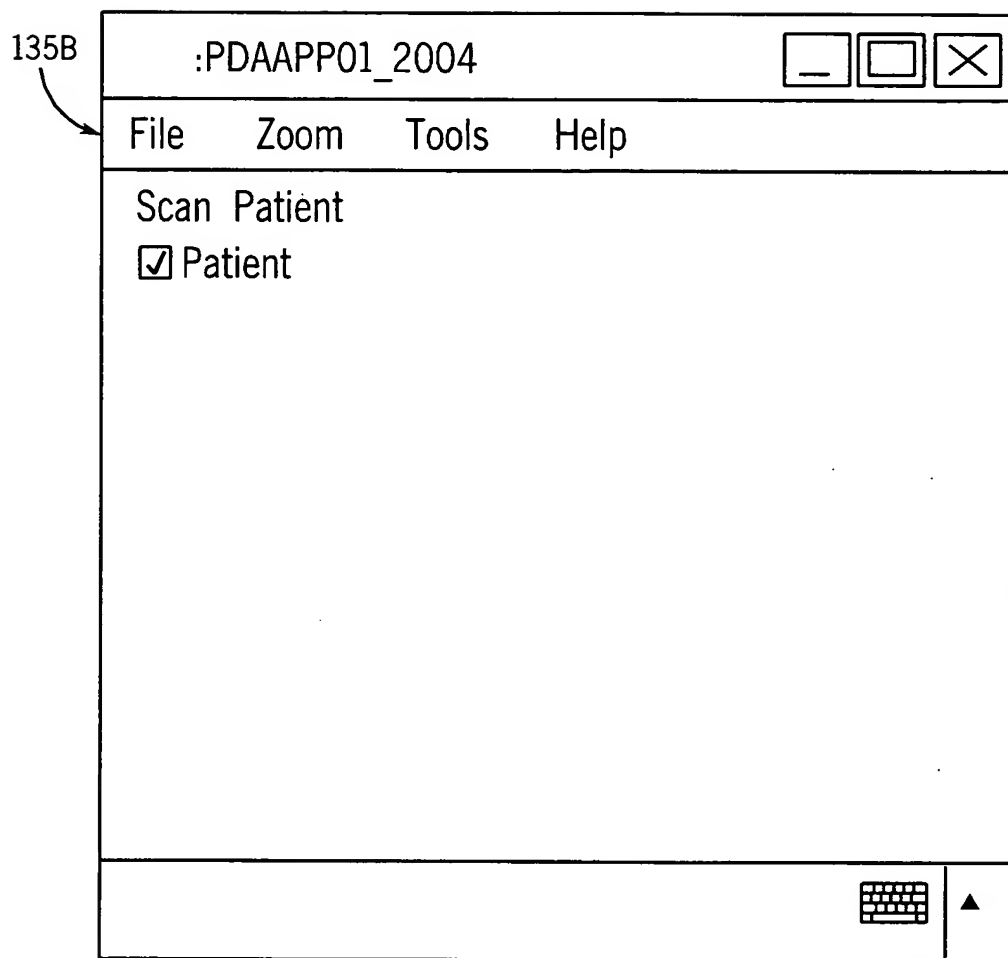


FIG. 9

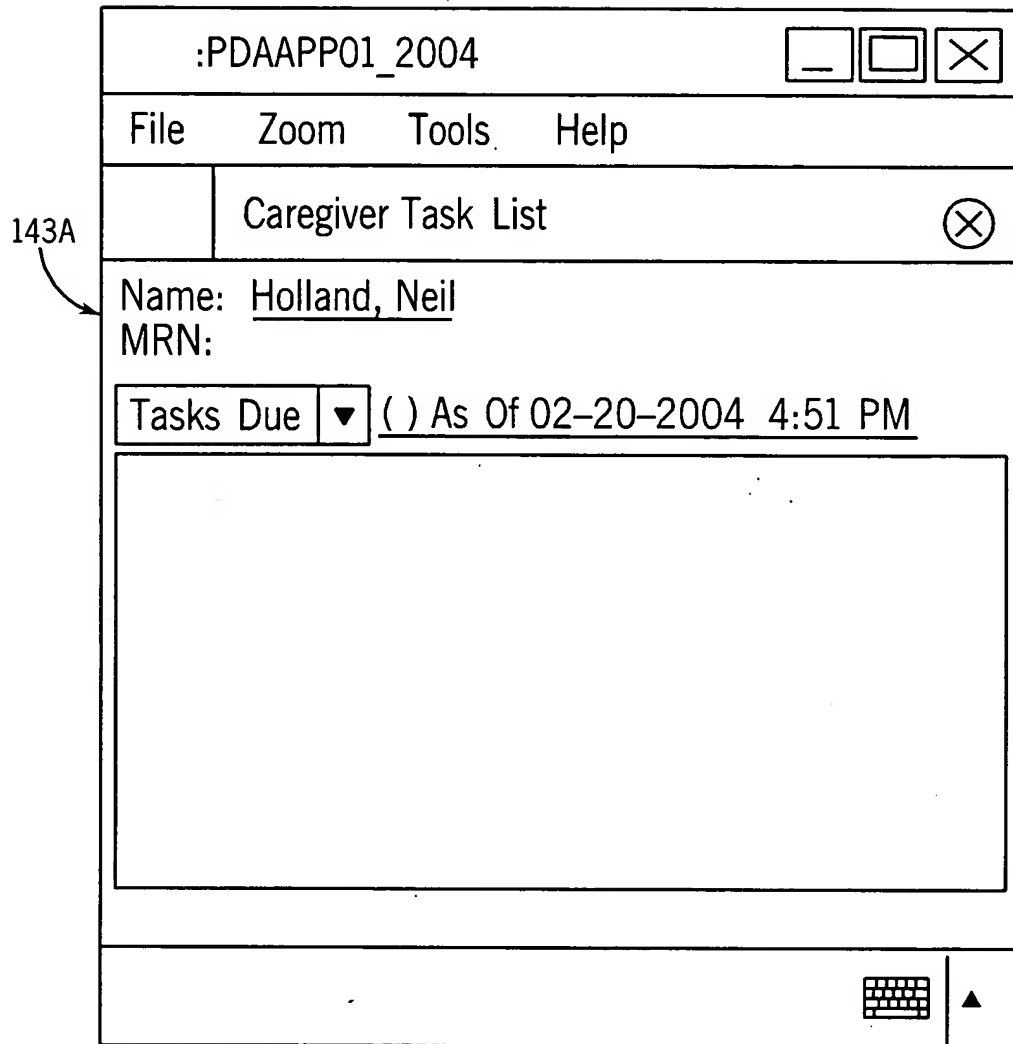


FIG. 10

143B

:PDAAPP01_2004

File Zoom Tools Help

Caregiver Task List

Name: Holland, Neil

NS 1000 mL

	Ordered	Pump
Perform Date	02-20-2004 ▼	
Perform Time	4:45:00 PM ▲▼	
Bag #	—	
Volume (mL)	1000	
Rate (mL / hr)	10	
Site		▼
Backpress	—	

Scan Pump Channel


Cancel Complete |  ▲

FIG. 11

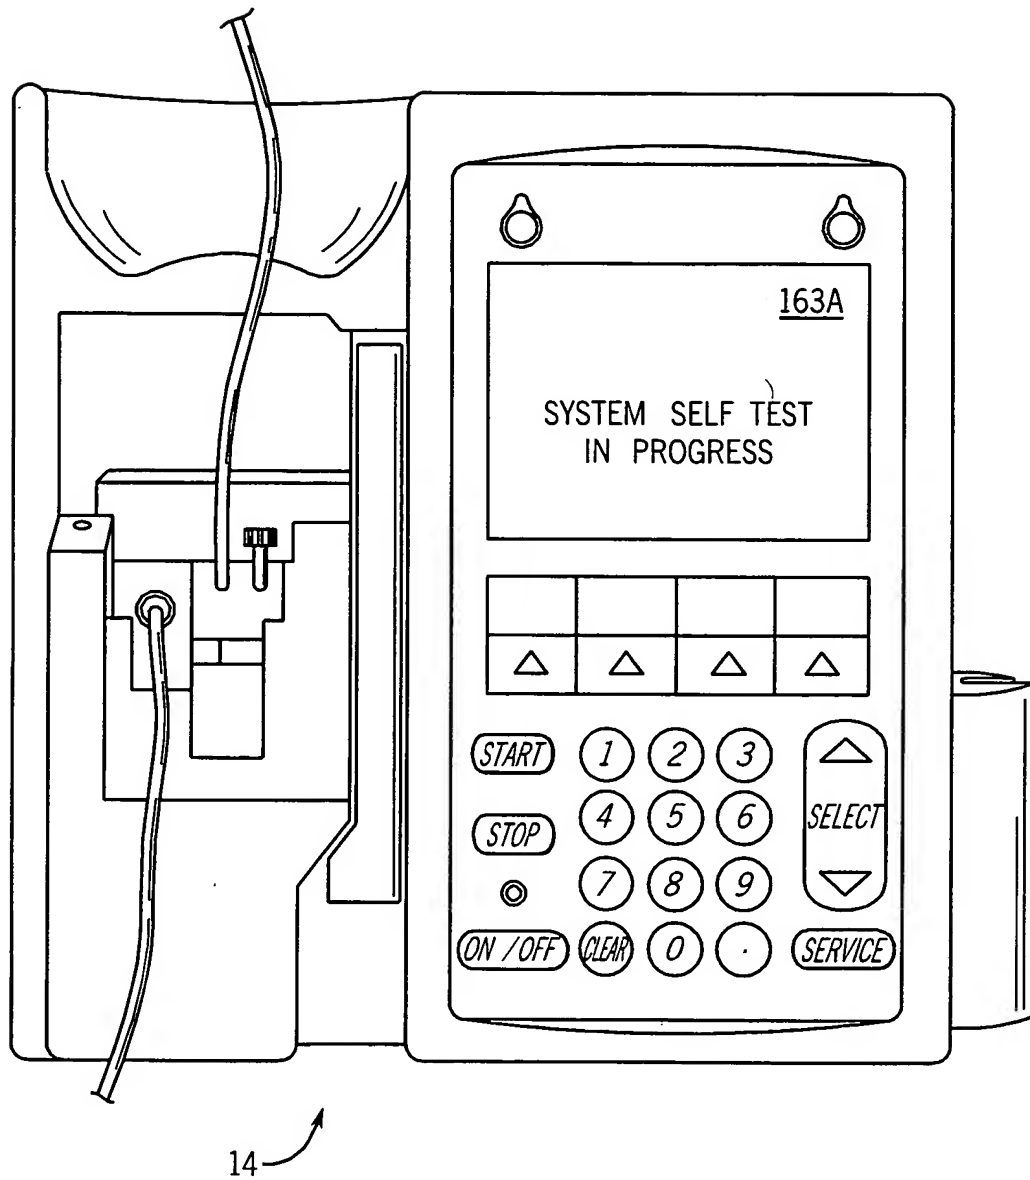


FIG. 12

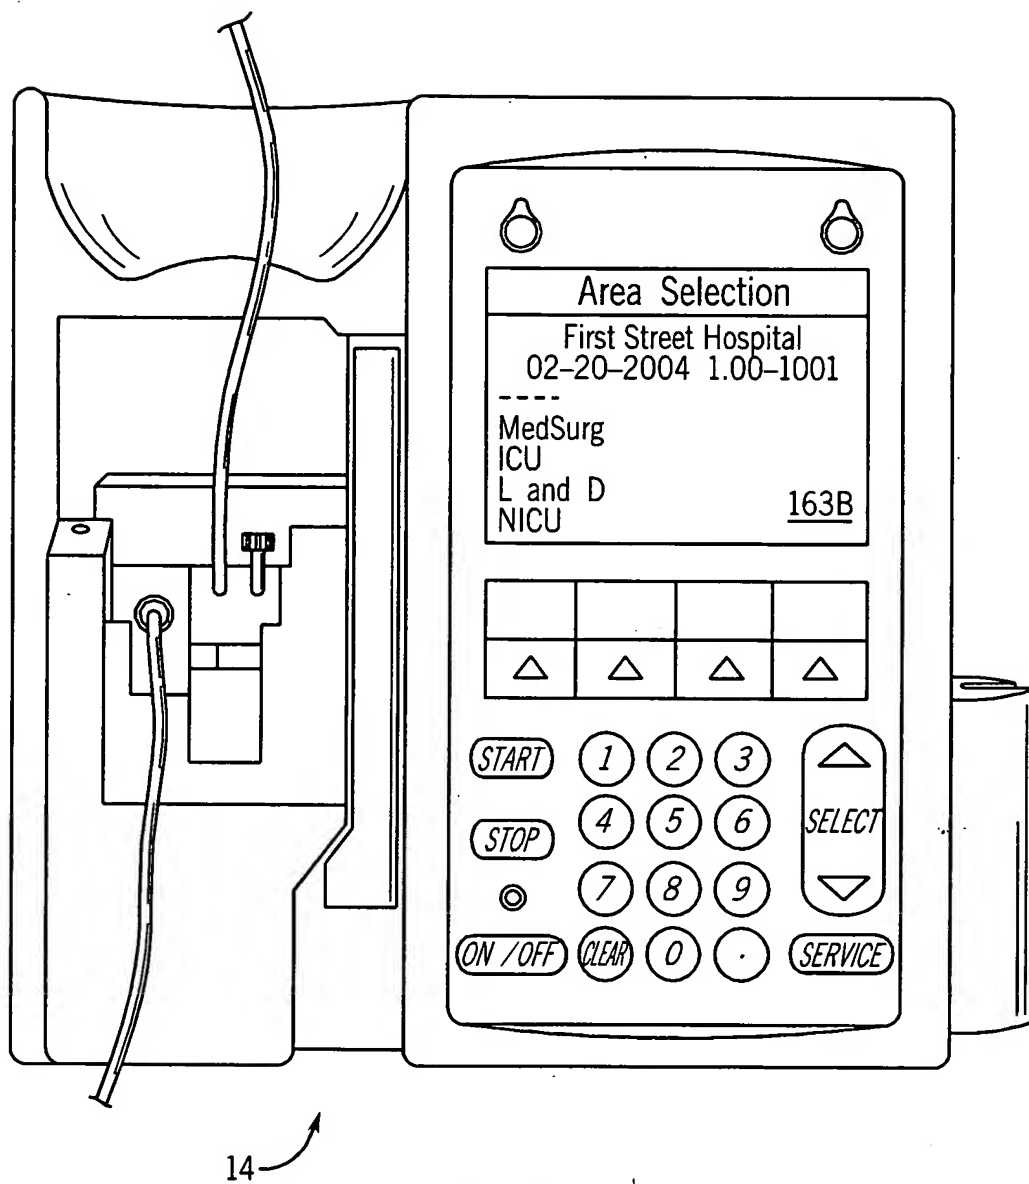


FIG. 13

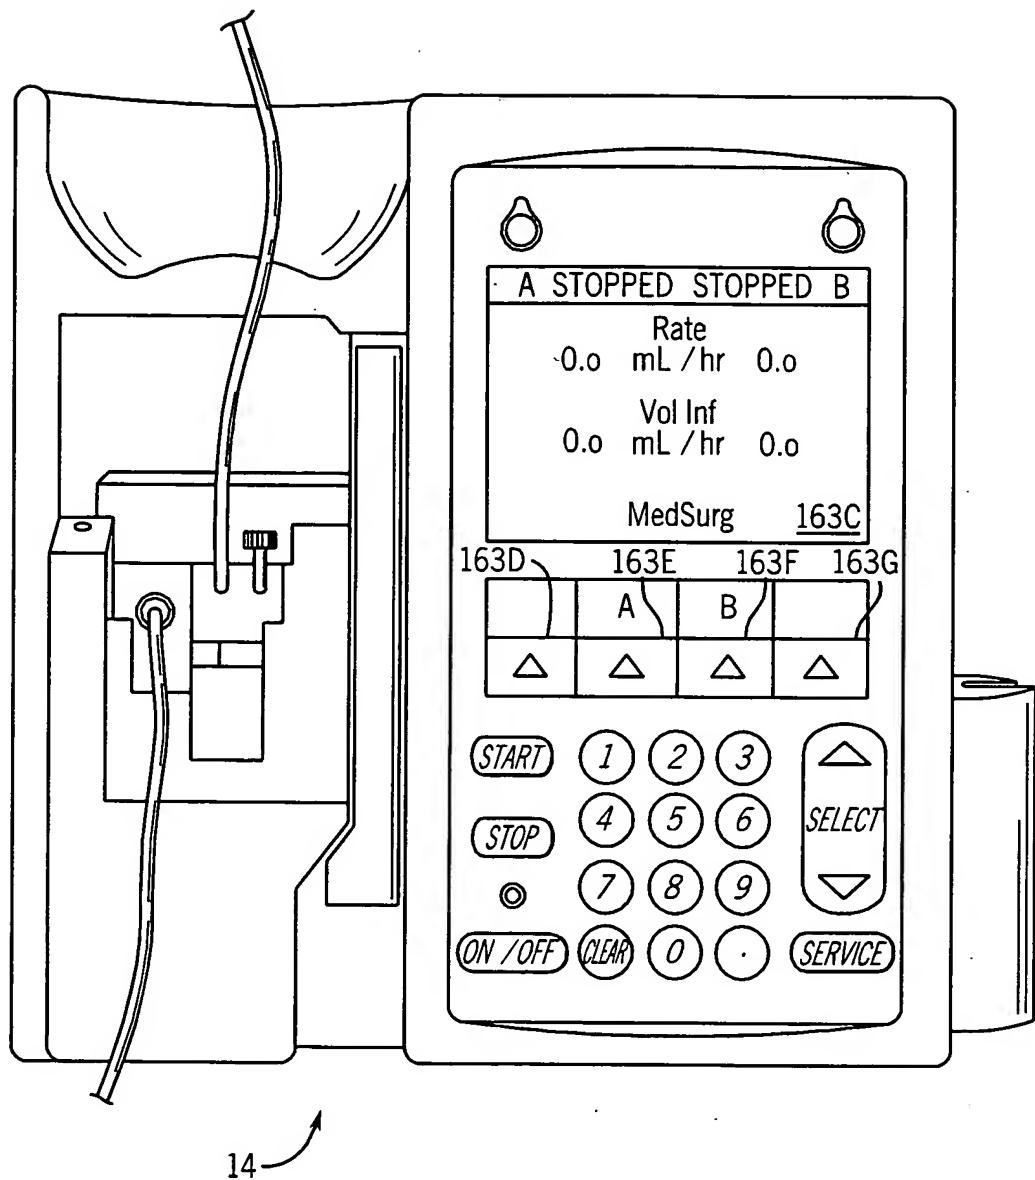


FIG. 14

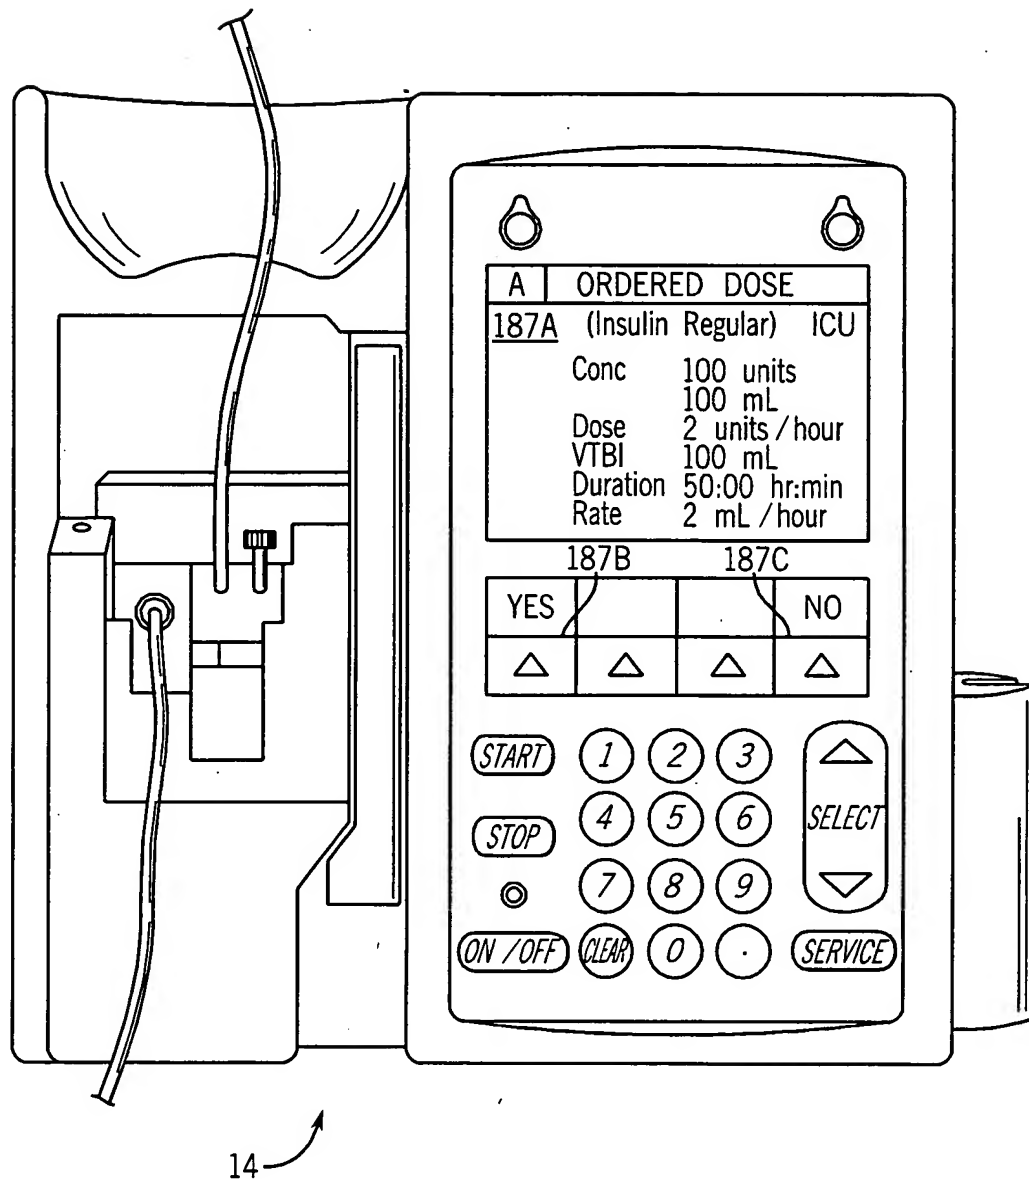


FIG. 15

:PDAAPP01_2004

File Zoom Tools Help

Caregiver Task List

191A Name: Holland, Neil

NS 1000 mL

	Ordered	Pump
Perform Date	02-20-2004 ▼	
Perform Time	4:45:00 PM ▲▼	
Bag #	—	
Volume (mL)	1000	1000.00
Rate (mL / hr)	10	10.00
Site		▼
Backpress	—	1.00

Pump Running

191C Cancel

191B Complete

▲

FIG. 16

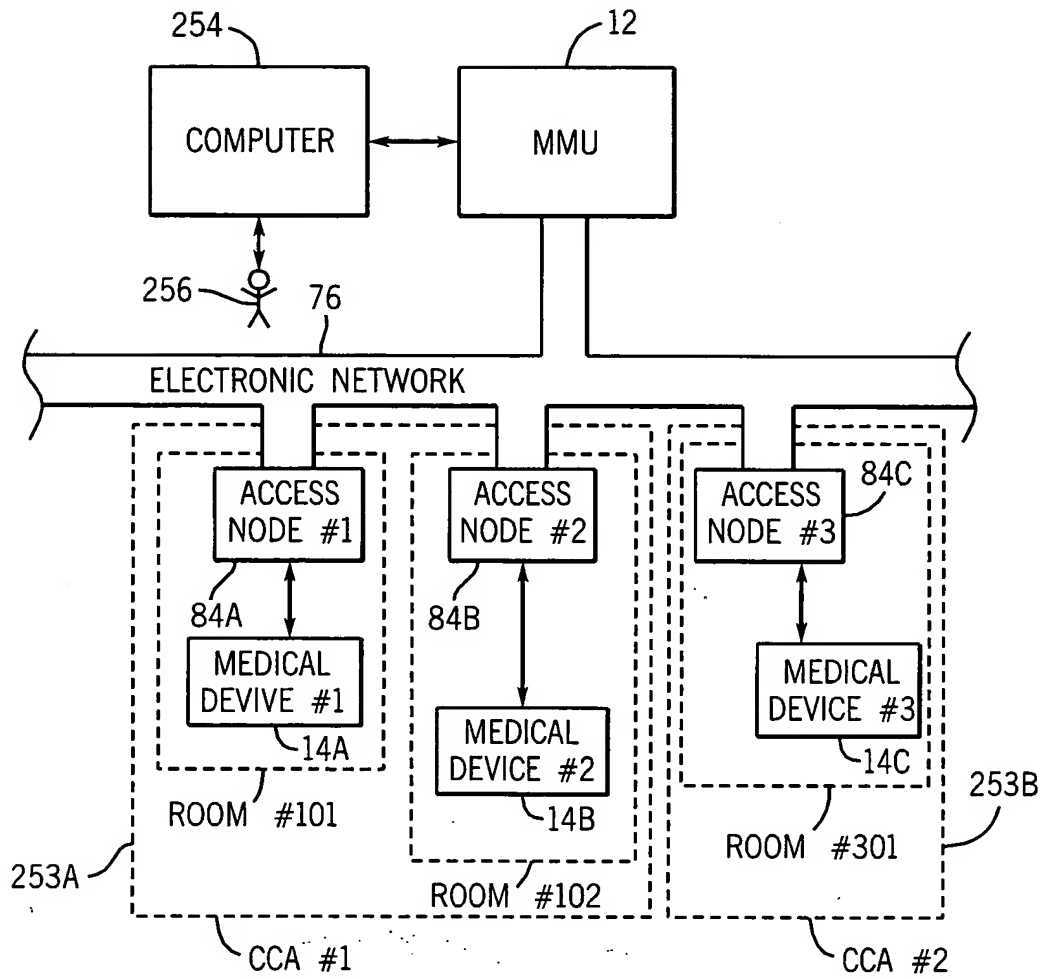


FIG. 17

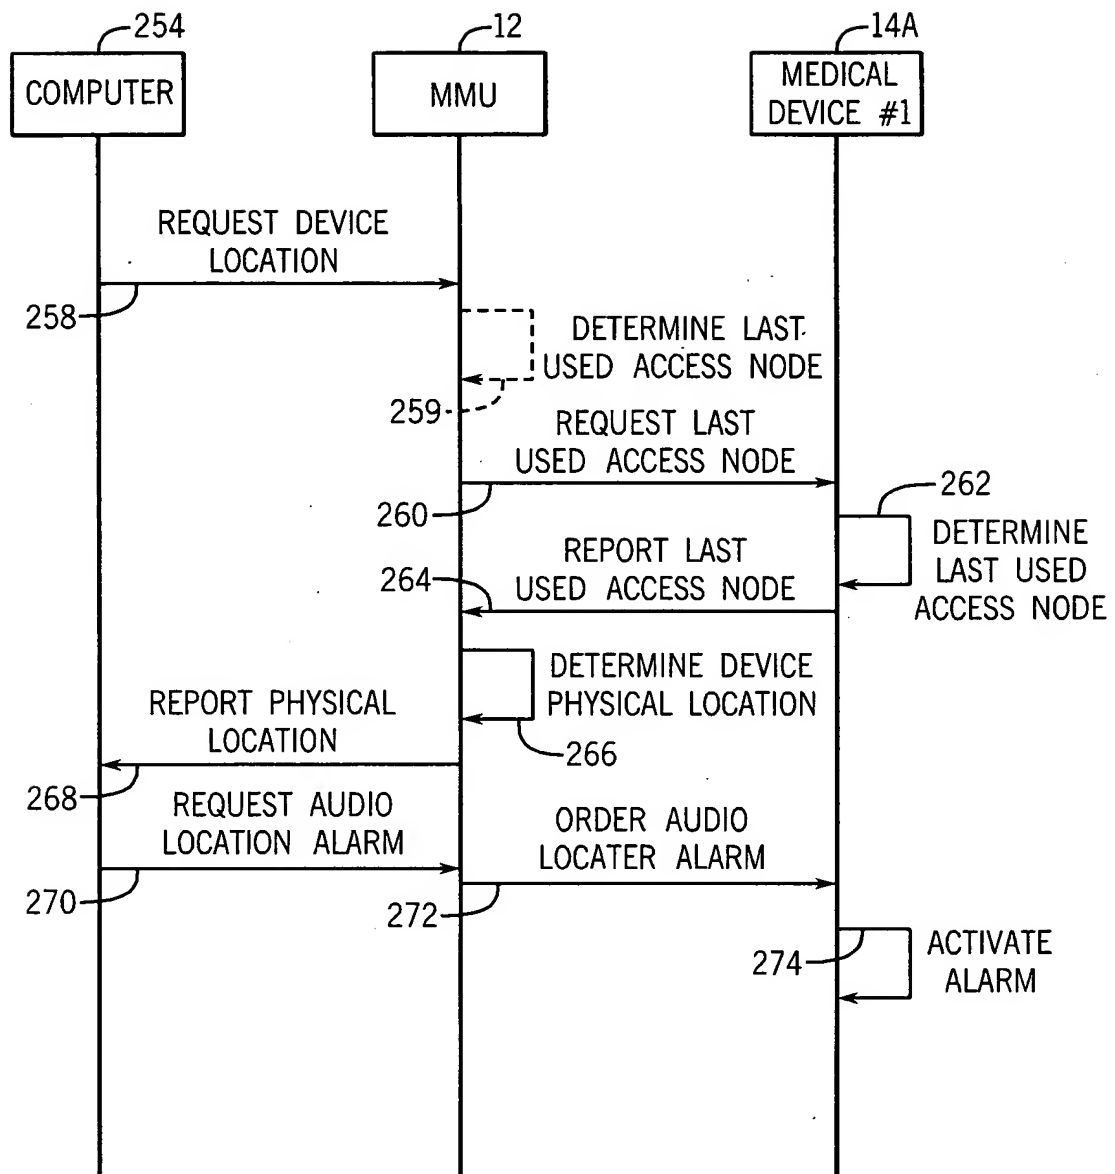


FIG. 18

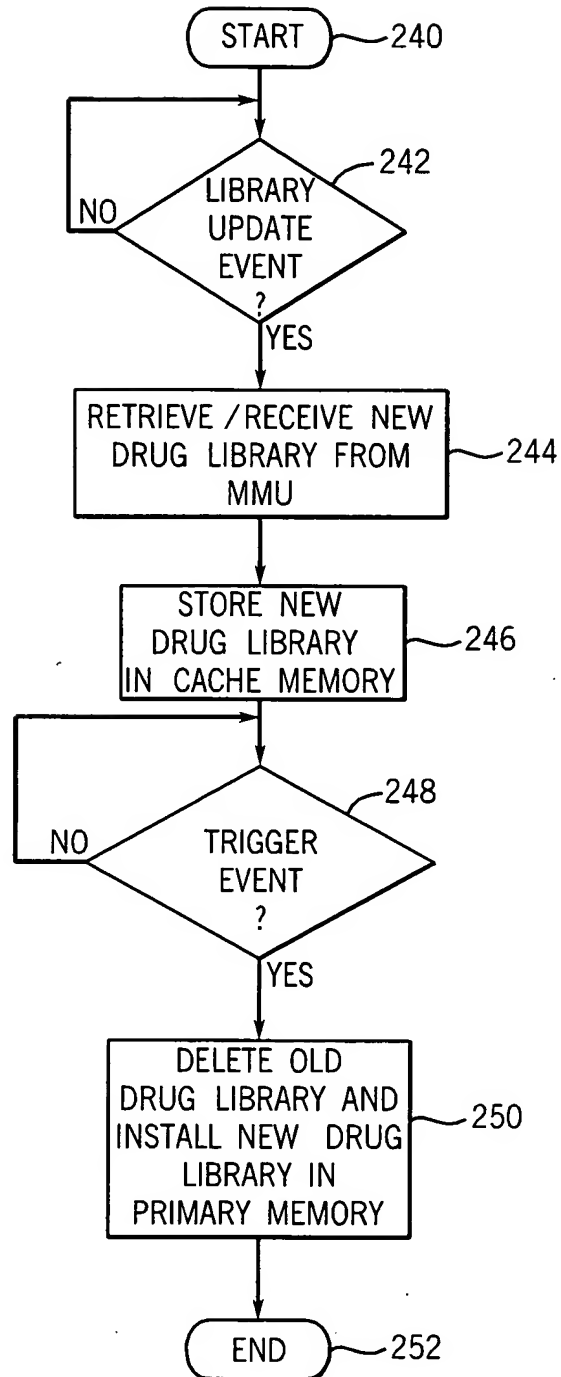


FIG. 19

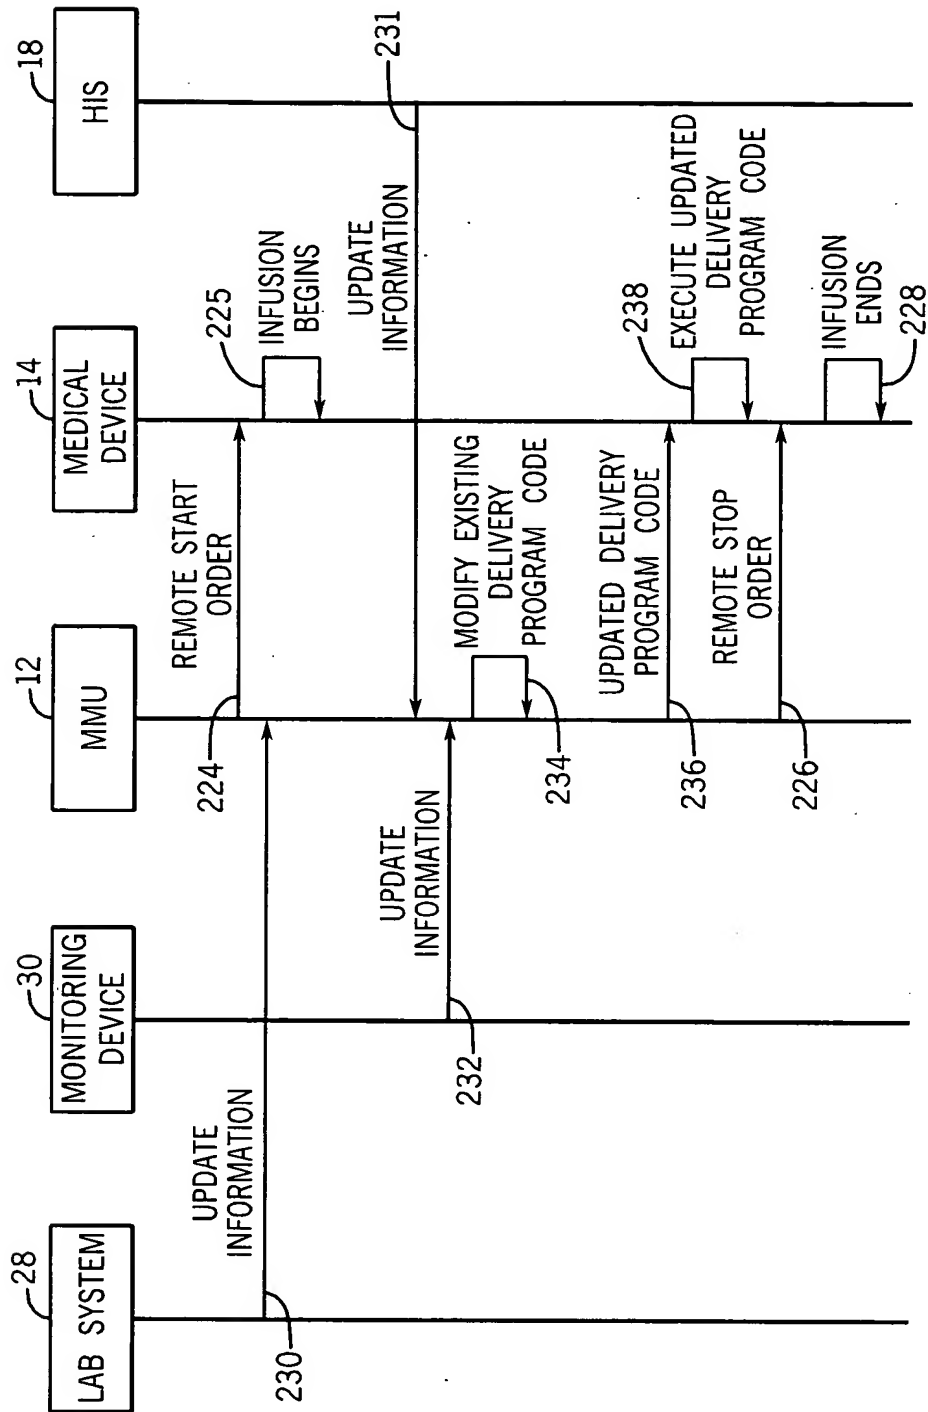


FIG. 20

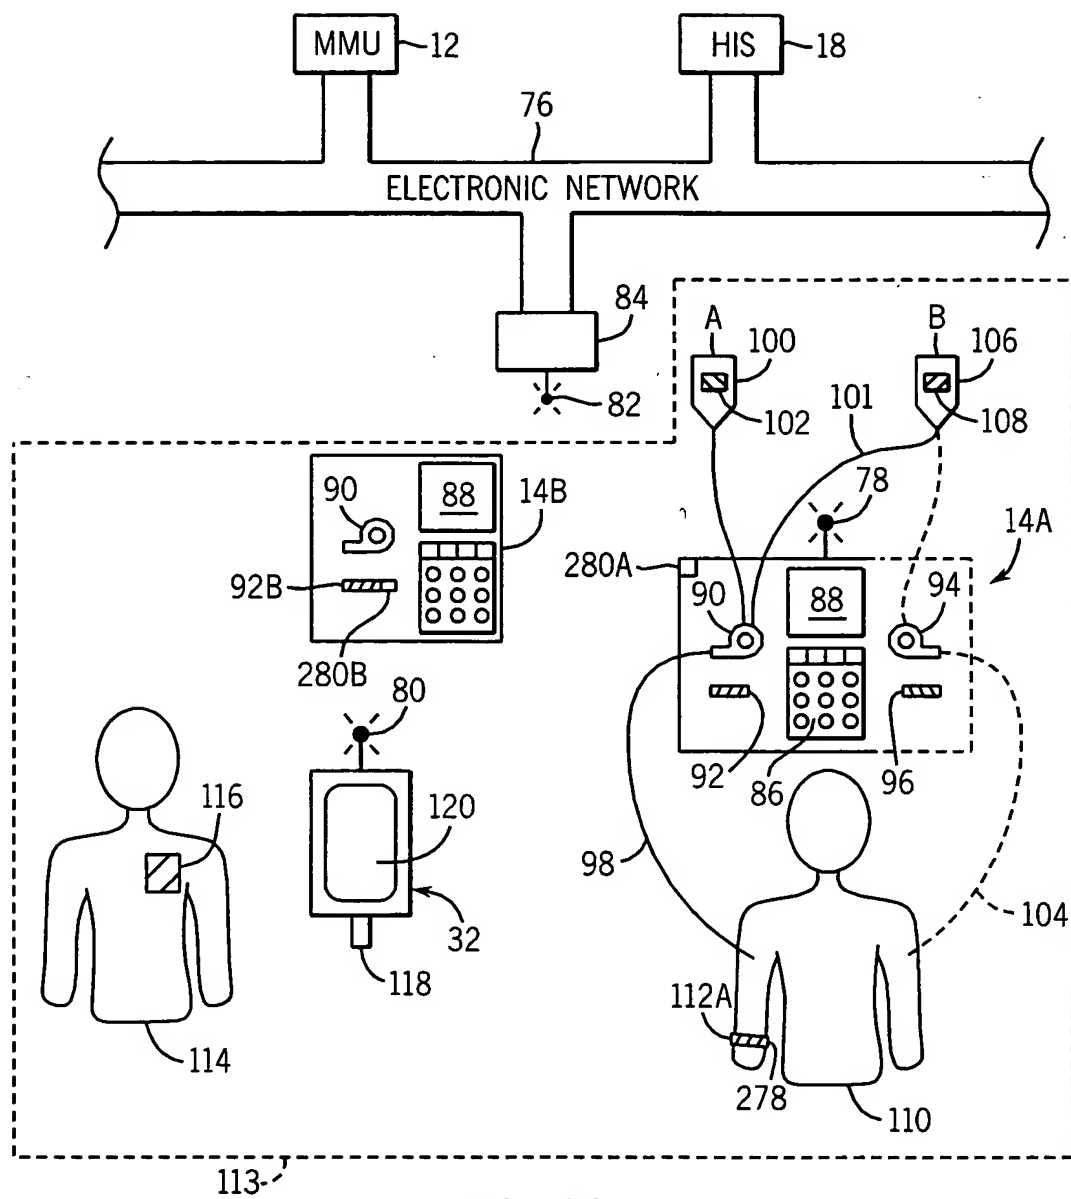


FIG. 21

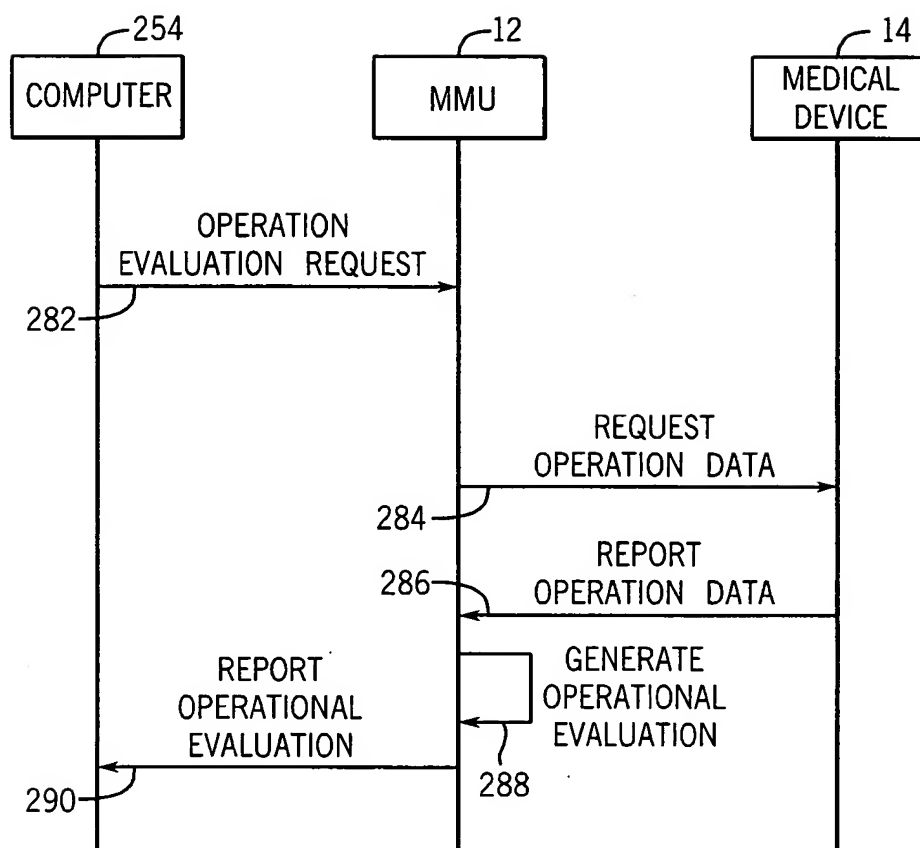


FIG. 22